


HAMEG Instruments

Measure time: 15:50:00

Measure date: 10.02.2017

CH1: 2,000V/DIV DC CH2: 2,000V/DIV DC TB A: 50 ms TR: CH2+AC PT: 25

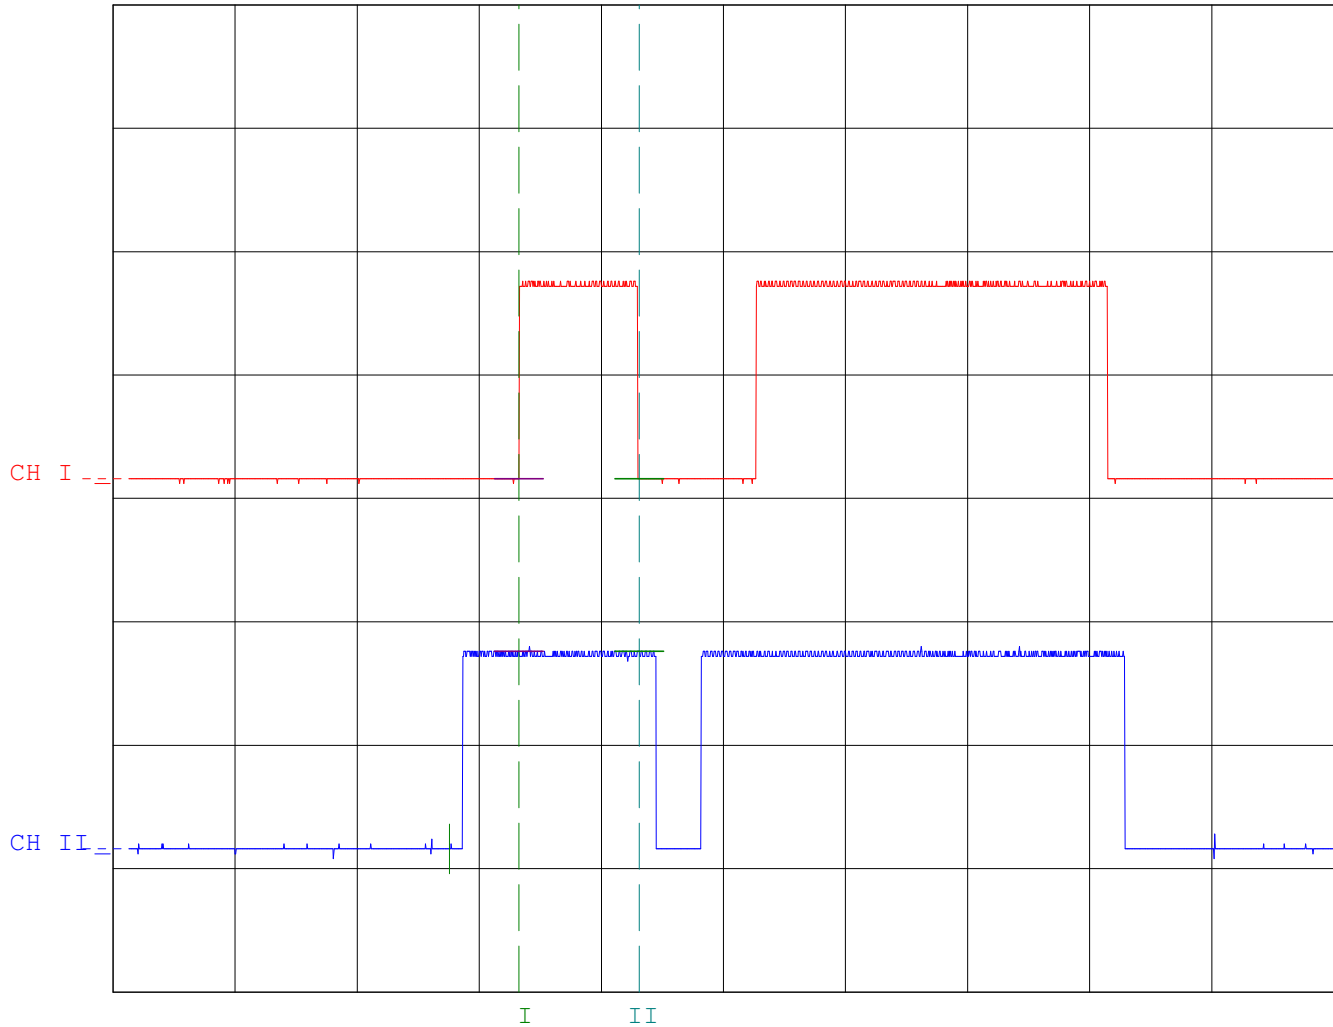

CH I : Cursor I: ,080V

Cursor II: ,080V

Diff. I-II: ,0000V

CH II: Cursor I: 3,280V

Cursor II: 3,280V

Diff. I-II: ,0000V

dt: 49,250 ms

1/dt: 20,305 Hz

Notes: