


HAMEG Instruments

Measure time: 16:50:05
Measure date: 10.02.2017

CH2: ,200V/DIV DC TB A: 10 ms TR: CH2+AC PT:-50

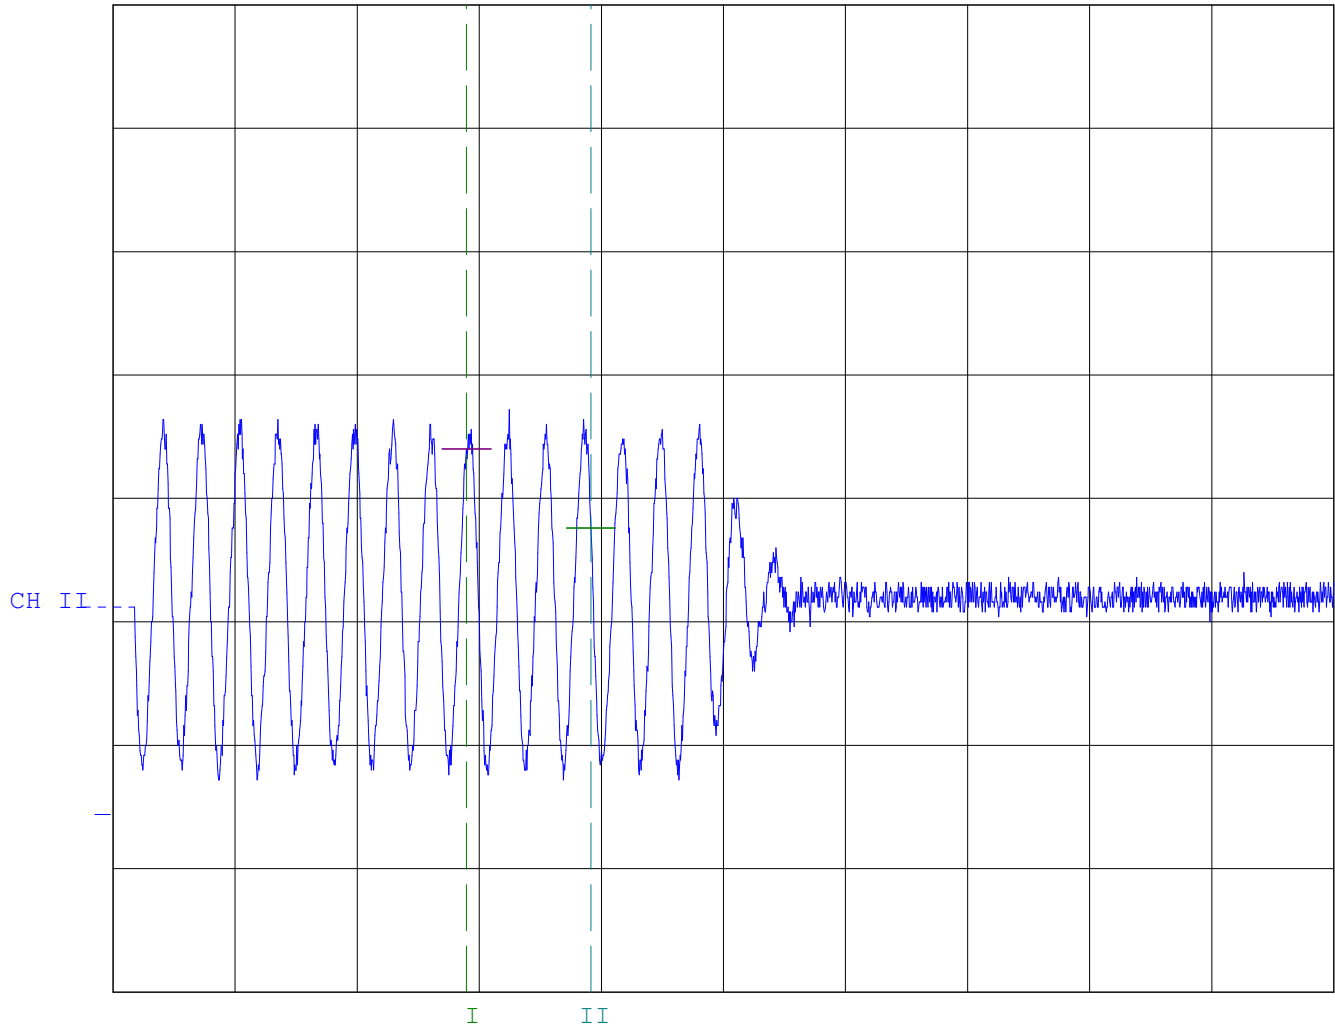

CH I : Cursor I: Off Cursor II: Off Diff. I-II: Off
CH II: Cursor I: ,592V Cursor II: ,464V Diff. I-II: ,1280V
dt: 10,200 ms 1/dt: 98,039 Hz

Notes: