


HAMEG Instruments

Measure time: 16:48:35
Measure date: 10.02.2017

CH2: ,200V/DIV DC TB A: 5 ms TR: CH2+AC PT: 25

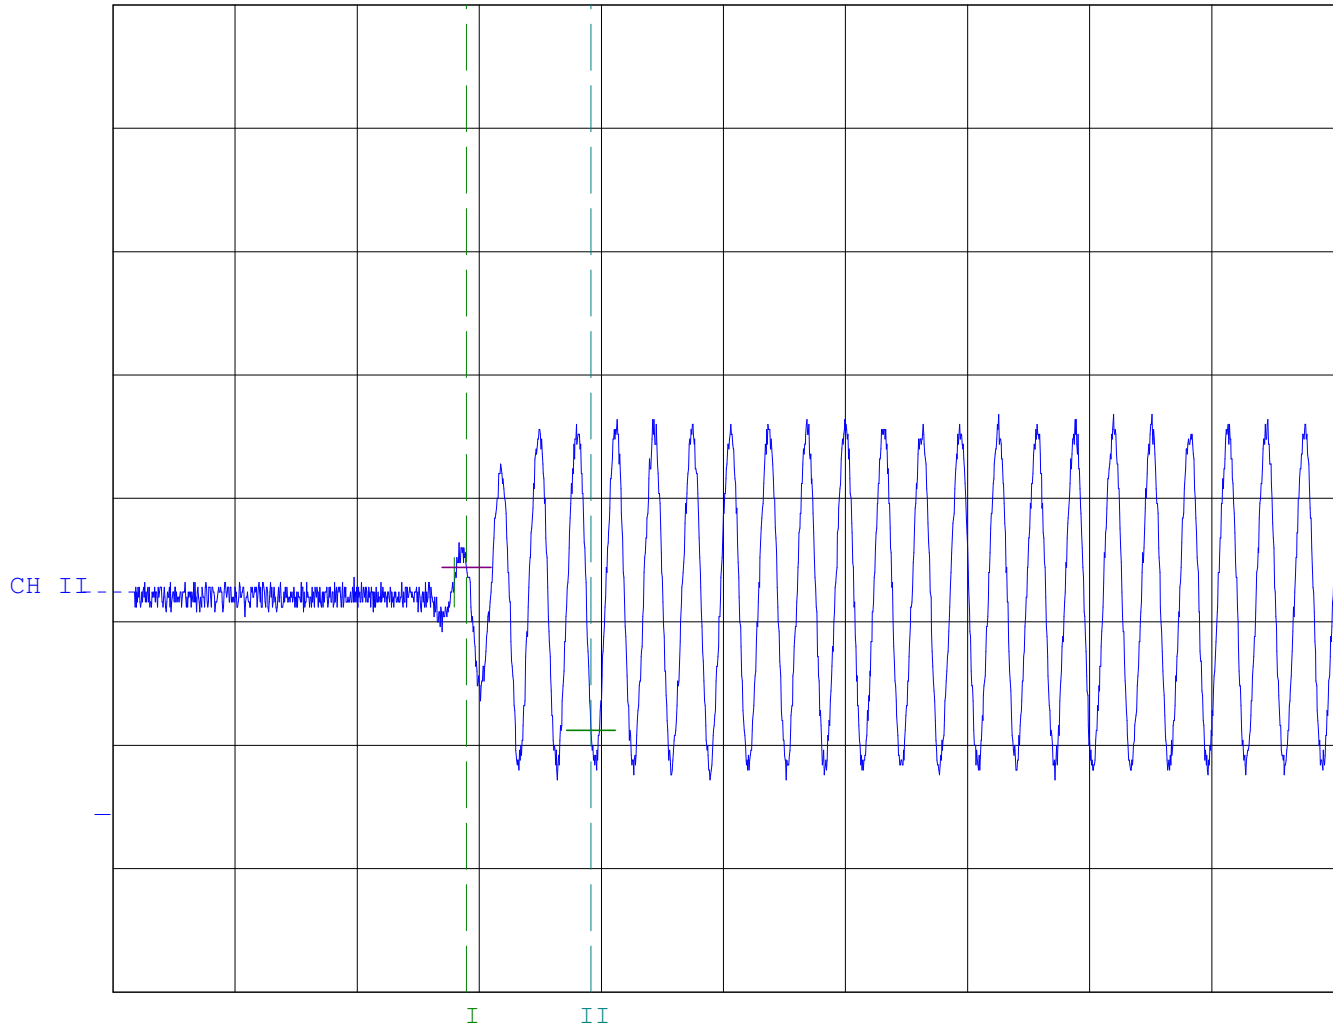

CH I :	Cursor I: Off	Cursor II: Off	Diff. I-II: Off
CH II:	Cursor I: ,400V	Cursor II: ,136V	Diff. I-II: ,2640V

dt: 5,100 ms 1/dt: 196,078 Hz

Notes: